

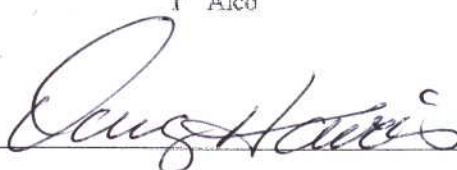
# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 04 2010

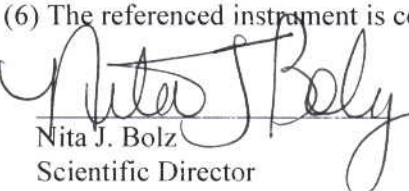
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130115 ✓
Name		DOUG E. HARRIS	ID# 5530 Date 3-2-2010 ✓
A	Agency	BRISTOL BAY POLICE	Phone # 907-246-4222
Instrument Location		BBPD BLDG 150 KSAFB KING SALMON AK ✓	
Alco S/N		X301605 ✓	Target Value 075 ✓ High Pressure
B	Alco Test Values		073 ✓ 1 <sup>st</sup> Alco 072 ✓ 2 <sup>nd</sup> Alco
Signature		 ✓	
(OVER)			

BMB  
3/18/2010

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 26<sup>th</sup> day of March, 2010.

  
(Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

